(51) International Patent Classification 5 :		(11) International Publication Number:	**WO 93/13711**
A61B 8/00	**A1**	(43) International Publication Date:	22 July 1993 (22.07.93)

(54) Title: METHOD AND APPARATUS FOR PROCESSING IMAGES
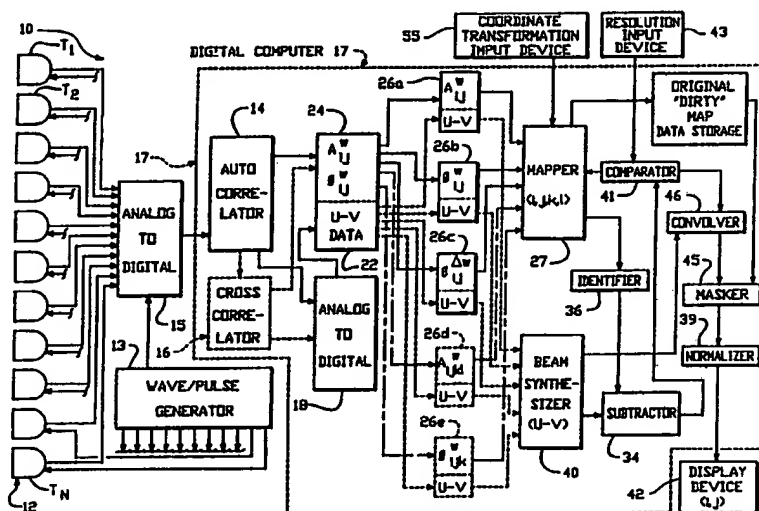
(57) Abstract

A method and apparatus for reducing noise and enhancing the dynamic range of an image data set gather from an array (12) of transducers (T). The method includes the step of processing the image data set in a digital computer (17) by a noise reduction technique, such as deconvolving the noise component by means of a CLEAN or other algorithm. Thereafter the artifact image data introduced by the noise reduction technique is reduced by masking the processed image data set with the original image data set. This masking is done by multiplying each data value in the processed image data set by the corresponding data value in the original image data set. The method further includes scaling and normalizing the masked data and finally displaying the same on an image display device (42). Additionally, for imaging apparatus (10) not having a cross-correlator (16), phase aberration is reduced by performing a coordinate transformation step prior to noise reduction using a non-standard set of coordinate transformation algorithms.

METHOD AND APPARATUS FOR PROCESSING IMAGES

TECHNICAL FIELD

The present invention relates, generally, to image
processing apparatus and methods of the type employed
5   in echographic applications, such as ultrasonic imaging,
sonar imaging, microwave imaging and radar imaging, as
well as in passive imaging such as is employed in radio
astronomy. More particularly, the present invention
relates to apparatus and methods for real-time imaging
10 of moving target objects and apparatus and methods which
employ image enhancing processing techniques, such as
deconvolution and near field or phase aberration
correction.

BACKGROUND OF THE INVENTION

15 Various linear and non-linear image processing techniques
have been extensively employed in radio astronomy, radar,
microwave and sonar applications to enhance the signal
to noise ratio (dynamic range) and clarity (resolution)

-2-

of images. Such systems typically have employed a plurality of transducers and/or receivers to create a synthetic aperture having many advantages over a single or filled aperture, but synthetic aperture systems also

5   inherently including significant noise components.

In radio astronomy applications, or interferometry, quite sophisticated non-linear signal processing techniques have been employed to reduce noise and enhance clarity. Among these techniques is deconvolution of the noise

10   component of image data from the valid signal component, and subsequent convolution of the signal components into a synthetic aperture image having greatly reduced noise and sharper resolution. Since radio astronomy is not concerned with real-time observations, quite elegant,

15   although   computer-burdensome,   signal   processing techniques can be employed to produce significant image enhancement.   R. Thompson, et al. Interferometry and Synthesis in Radioastronomy, J. Wiley, 1986.

In applications which will benefit from a substantially

20   real-time display of images, particularly of moving targets, the computing burden of conventional radio astronomy signal processing techniques is too great. In my above-identified co-pending application, I have recently adapted and employed certain interferometry

25   signal processing techniques to ultrasonic echographic imaging.   These   imaging   processing   techniques,   as employed in biomedical ultrasonic imaging, are more fully described in my prior applications identified above, which are incorporated herein by reference.

30   Noise deconvolution involves taking an original image data set from an array of transducers or receivers, deconvolving or mathematically separating the noise component side lobe data from the true image data using non-linear algorithms. The original or noise-containing

-3-

data is sometimes referred to as a "dirty" image data set. It is known, for example, that side-by-side transducers or receivers will receive image data from a point source which would produce an image map having

5   side lobes or noise produced by incompleteness of the synthesized aperture. For any array of a plurality of receivers or transducers, therefore, there will be a characteristic beam pattern (power pattern) or "point spread function" for the array. The beam pattern or

10   point spread function is the image which would be sensed by the array if a single point were the only target in the image field; it does not, however, resemble a single point. Since there are a plurality of side-by-side transducers or receivers in the array making up the

15   synthetic aperture, many of the receivers in the array may "see" the point source to some degree and as a result, the image will not be a point, but a spreading and distortion of the point including side lobes. As the image being processed becomes more complex, with

20   multiple valid targets, the effects of side lobe noise become more pervasive and complex, and removal of these noise effects from the image data for the synthesized aperture becomes more important.

The elimination of noise using deconvolution may proceed

25   by selecting the brightest or highest intensity data point on the "dirty map" of the image and then deconvolving this noise from the valid image data by using an algorithm based upon the point spread function or the characteristic beam pattern. Thus, one assumes

30   that for the given brightest point, the side lobes, or noise, inherent to a multiple transducer array, should be removed. All of the data points, other than the brightest point, which would contain noise or side lobe effects from the brightest point, have their respective

35   intensities reduce by an amount determined by the beam pattern or point spread function. The removal of the

-4-

beam pattern, therefore, has the effect of removing the side lobes from data throughout the map.

Once noise around the brightest data point has been removed, the deconvolution process then proceeds to the
5 next brightest data point in the dirty map, assumes that this next brightest data point is a valid data point and then removes the corresponding beam pattern for such data point from the remainder of the map. This process continues until the intensity of the brightest data point
10 from which the noise is deconvolved reaches a predetermined level, for example, ten percent, of the intensity of the brightest data point in the entire map.

The beam pattern or point spread function is a three-dimensional pattern with the amplitude being the data
15 intensity or the height dimension. The deconvolution process in which the side lobes are removed, therefore, ideally and in radio astronomy is a three-dimensional process.

Radio astronomy, however, has the luxury of not been
20 needing to process the signals on a real-time basis since the objects essentially are stationary from the point of view of the receivers. Additionally, substantial computing power can be dedicated to the signal processing task. As used herein, the expression "real-time" shall
25 be understood to mean imaging at a rate of at least about 15 images (complete data maps) per second and preferably between about 30 to about 60 images per second. In some application real-time is considered to be as low as 5 images per section but this would be acceptable only for
30 relatively slow moving targets.

The result in radio astronomy has been that relatively elegant and more accurate algorithms can be employed to accurately subtract the point spread function or beam

-5-

pattern by deconvolution of the noise from the signal.
Thus, three-dimensional CLEAN algorithms can be used,
as can three-dimensional hybrid mapping and maximum
entropy algorithms.   Maximum entropy is generally
5   regarded as being the most accurate algorithm, but is
also has the greatest computational burden.

Typically, in ultrasound imaging, images are displayed
on a video display terminal in which there are up to 512
lines with 512 pixels per line.   A data map will,
10   therefore, include up to 262,144 pixels or data points.
In real-time imaging each map is presented 15 to 60 times
per second.   As will be appreciated, any deconvolution
system which scans all the data points prior to making
a selection as to the brightest point, will be faced with
15   a computational burden which is substantial and which
will make real-time imaging with an apparatus of
reasonable cost very difficult.

It is also known, however, that deconvolution processes
inherently introduce data into the processed image data
20   set which is not valid or does not actually represent
the object being imaged. These processing induced data
are known as image processing "artifacts," and while they
are far fewer than the noise data which has been
eliminated by deconvolution, they degrade the image and
25   particularly image resolution and produce inaccuracies
which may compromise interpretation of the image.

As the deconvolution algorithms get more sophisticated
and complex, the number and effects of processing
artifacts are reduced, but the computational burden and
30   time required are increased.   As assumptions,
simplifications and less sophisticated algorithms are
employed, real-time processing becomes more realistic,
but image degradation from processing artifacts becomes
more significant.

-6-

Radio astronomy imaging routinely employs cross-correlation of data to produce useful data sets prior to deconvolution. While ultrasonic imaging literature suggests application of cross-correlation to ultrasonic

5   imaging, commercially available ultrasonic imaging apparatus has no provision for data cross-correlation. This is particularly important in that one of the significant sources of image noise is the inhomogeneous medium through which image signals pass. In radio

10 astronomy the medium is miles and miles of atmosphere and the distortions or noise produced by the same is called the "near field effect." In ultrasonic imaging the inhomogeneous medium is human tissue, and the distortion or noise produced is referred to in the

15 industry as "phase aberration."

In radio astronomy imaging the near field effect is completely removed by employing closure phases obtained from the cross-correlation data prior to deconvolution of the noise. In ultrasonic imaging various alternative

20 approximations have been employed to try to minimize or reduce near phase aberration. See, e.g., U.S. Patent Nos. 4,817,614 to Hasler et al. and 4,835,689 to O'Donnell which employ adaptive reduction of phase aberrations.   See also, e.g., companion technical

25 articles, O'Donnell et al. "Phase Aberration Measurements in Medical Ultrasound: Human Studies", Ultrasonic Imaging, Vol. 10, pp. 1-11 (1988); O'Donnell et al. "Aberration Correction without the Need for a Beacon Signal", IEEE Ultrasonics Symposium, pp. 833-837 (1988);

30 O'Donnell et al., "Phase-Aberration Correction Using Signals from Point Reflectors and Diffuse Scatterers: Measurement",   IEEE Transactions on Ultrasonics, Ferroelectrics and Frequency Control, Vol. 35, No. 6, pp. 768-774 (1988). See, also, Hayakawa "Multifrequency

35 Echoscopy for Quantitative Acoustical Characterization of Living Tissues", J. Acoustical Society of America,

-7-

Vol. 69 (6), pp. 1838-1840 (1981) where an approximation
of the attenuation coefficient in human tissue is
developed.

5   In an article by Somer et al., "Real-Time Improvement
of both Lateral and Range Resolution by Optical Signal
Processing", Ultrasonics Symposium Proceedings,
pp. 1002-1005 (1977) an ultrasonic image enhancing
process is described in which lateral and axial
resolution is improved by using coherent optical
10 filtering. This is an optical approach to achieve an
approximate phase aberration correction.

In U.S. Patent Nos. 4,604,697 and 4,553,437, both to
Luthra et al., a hybrid image is produced from the vector
addition of amplitude and phase data from an array of
15 transducers at a plurality of frequencies. The overall
image is produced by adding partial images. In U.S.
Patent No. 4,586,135 to Matsumoto side lobe reduction
is employed utilizing phase data to provide a holographic
data set for reconstruction by a synthetic aperture
20 technique.

Auto and cross-correlation also have been suggested in
U.S. Patent No. 4,397,006 to Galbraith to determine
digital time domain filter parameters for noise reduction
in seismographic teachings.

25 I have pointed out in my earlier copending application
that by using cross-correlation in ultrasonic imaging
and combining the same with specific image processing
techniques phase aberration can be completely eliminated.
Since present commercially available ultrasonic equipment
30 does not include a cross-correlation capability, however,
this approach is not currently easily implemented as an
ultrasonic image enhancing process, particularly when
retro-fitting existing ultrasonic equipment.

-8-

Thus, as phase aberration approximations are employed in ultrasonic imaging, the number of processing artifacts is increased.

Still other attempts have been made to enhance the clarity or resolution of ultrasonic images, but only limited success has been achieved. In U.S. Patent No. 4,478,085 to Sasaki, the thickness of the ultrasonic transducers was varied over the array to try to minimize beam expansion. U.S. Patent No. 4,470,305 to O'Donnell employs an annular array of ultrasonic transducers and time delayed pulses to simulate a horn transducer having a sharp focus in the near field. Using this system improved focusing can be achieved up to 20 centimeters, but imaging is accomplished at 3 MHz. The improvement in focus at depth is accomplished in the O'Donnell patent by using variable received signal gains to try to reduce the side lobe noise in the images.

In U.S. Patent No. 4,677,981 to Coursant, improvement in the ultrasonic echographic image focusing is attempted by using polarization characteristics of the ultrasonic transducers. The disadvantage of this approach is the absence of the initial polarization information and a lack of total intensity. This approach adds little to significantly improve dynamic range and resolution of the ultrasonic images.

Variable frequency ultrasonic scanning also has been used, e.g., U.S. No. 4,442,715 to Brisken et al., and pitch variation is employed in the device of U.S. Patent No. 4,664,122 to Yano. Doppler shift also has been employed to detect motion of scanned targets, for example, as is taught in U.S. Patent No. 4,509,525 to Seo.

-9-

In a published abstract of a paper that was not given
or published, Dr. Nathan Cohen suggested that in
underwater acoustic imaging linear and nonlinear imaging
techniques could be used to aid in recovery of phase
5   observables for increased dynamic range and image
accuracy. The abstract also suggested that techniques
from imaging disciplines such as optics and radio
astronomy might be applied. Cohen, "Phase Recovery and
Calibration with Underwater Acoustic Arrays", J.
10   Acoustical Society of America, Sup. 1, Vol. 82,
pp. 574-575 (1987). The techniques which might be
applicable, how they might be applied and their
suitability for medical imaging is not set forth in the
abstract.

15   While radio astronomy images are displayed in Cartesian
coordinates as X.Y images, ultrasonic images are more
conventionally displayed in polar coordinates. Thus,
a sector-like ultrasonic image is displayed in which the
apex of the image is located at the transducer array.
20   The data are displayed in a range or radius, r, and an
azimuth or angle, θ, format.

When an r,θ display format is used, the noise and side
lobes at increasing range from the transducer will appear
larger in extent. The image at increasing ranges appears
25   much noisier than at ranges close to the transducer.
In order to deconvolve the beam noise for an r,θ format
display, a coordinate transformation of the r,θ data to
X,Y coordinates for deconvolution in the X,Y format
usually is performed. It also would be possible to
30   convert the X,Y point spread function into r,θ format
and then deconvolve the noise and in an r,θ format for
conventional display.

The process and apparatus set forth in my prior copending
application does not eliminate noise in the form of

-10-

signal processing artifacts, nor is phase aberration
reduced for signal processing equipment which does not
include a cross-correlator. Both these goals are highly
desirable, particularly if they can be accomplished at
5   real-time rates with apparatus which can be retrofit to
existing equipment at only modest cost.

Accordingly, it is an object of the present invention
to provide an image processing method and apparatus which
is capable of substantially reducing and even eliminating
10   image processing artifacts produced by nonlinear and
linear image processing techniques.

It is a further object of the present invention to
provide an image processing method and apparatus which
is capable of producing images having enhanced dynamic
15   range and only a modest increase in computational burden.

It is another object of the present invention to provide
an echography apparatus and method which will generate
high-resolution images, at real-time imaging rates, of
stationary and moving target objects in an inhomogeneous
20   medium using ultrasonic signals.

Still a further object of the present invention is to
provide an ultrasonic imaging apparatus and method which
can retrofit to and is usable with existing ultrasonic
transducer   arrays   and   correlators   to   enhance   the
25   resolution and dynamic range of the images produced.

Still another object of the present invention is to
provide an image processing apparatus and method in which
phase aberration can be reduced.

Another object of the present invention is to provide
30   an echographic image processing apparatus and method
which is capable of real-time image processing with

reduced phase aberration and reduced processing-induced
noise, and which has modest cost and can be easily
retrofit for use with a variety of echographic imaging
apparatus.

5   Still another object of the present invention is to
provide an image processing apparatus and method which
can be easily adjusted by medical personnel to
empirically reduce phase aberration.

The apparatus and method of the present invention have
10 other features of advantage and objects which will become
apparent from, and are set forth in more detail in the
following Best Mode of Carrying Out the Invention and
the accompanying drawing.

DISCLOSURE OF INVENTION

15 In one aspect of the present invention a method and
apparatus for enhancing processed image data to remove
processing artifacts is provided. The method comprises,
briefly, the steps of comparing data from a processed
image data set with corresponding data from an original
20 or relatively unprocessed image data set, and revaluing
data in the processed image data set in proportion to
the value of corresponding data in the original image
data set. The apparatus includes, briefly, "masking"
apparatus connected to reduce the value of data in
25 processed image data set by an amount determined by the
data in an original image data set.

In another aspect of the present invention, a method and
apparatus for reducing phase aberration is provided.
The method is comprised, briefly, of the steps of
30 performing a non-standard coordinate transformation on
one of data from an image data set and a deconvolution
algorithm used to deconvolve noise from image data. The
non-standard coordinate transformation can be empirically

adjusted by a clinician to reduce phase aberration without the use of cross-correlation apparatus. Phase aberration apparatus including a coordinate transformation input device coupled to vary coordinate
5 transformation from conventional algorithms is provided.

BRIEF DESCRIPTION OF THE DRAWING
FIGURE 1 is a schematic representation of echographic image processing apparatus constructed in accordance with the present invention.

10 FIGURE 2A is a graphical representation of a plot of image data as it would appear in memory at various stages of signal processing using the method of my prior application.

FIGURE 2B is a graphical representation of a plot of the
15 same image data as FIGURE 2A using the signal processing method of the present application.

FIGURE 2C is a graphical representation of the same image data as FIGURE 2A as it should appear in memory at the stage immediately before display.

20 FIGURE 2D is a "Data Key" for the symbols used in FIGURES 2A-2C.

BEST MODE OF CARRYING OUT THE INVENTION
The apparatus and process of the present invention for removing signal processing artifacts is described in
25 detail in connection with a side lobe subtraction process using a CLEAN algorithm, but it will be understood that the present invention has application to a wide range of signal processing techniques which are capable of generating data artifacts. Thus, the system of the
30 present invention is applicable to hybrid mapping techniques, maximum entropy noise reduction techniques,

-13-

and even linear signal averaging processes. Similarly,
the system of the present invention is described in
detail in connection with ultrasonic signal processing,
but it is applicable to active image processing systems
5   employed in radar, microwave, sonar and optical signal
processing, as well as being applicable to passive signal
processing of the type used, for example, in radio
astronomy.

As shown schematically in FIGURE 1 an ultrasonic
10   echography imaging apparatus, generally designated 10,
can be seen to include a transmitting and receiving
transducer array, generally designated 12, which includes
transducers T_1 through T_N.   Transducers   T   are
geometrically positioned to transmit a signal in the
15   direction of a target object (not shown), such as human
tissue. In radar, microwave and other applications the
target object can vary substantially, and the nature of
the target object does not form a portion of the present
invention. The greater the number of transducers, the
20   larger the geometric aperture of the image which can be
obtained from array 12. Transducers T need not be
positioned in a linear array as shown in FIGURE 1, and
more conventionally the transducers will be mounted in
a two-dimensional array on a common frame or probe at
25   predetermined fixed relative locations.

In ultrasonic applications it is preferable that
transducers T_1 through T_N each transmit a broad band pulse
or Doppler-shifted continuous wave signals. Thus,
wave/pulse generator 13 is electrically coupled to each
30   of transducers T to drive the same and further is coupled
to an analog-to-digital converter 15 for input to a
general purpose digital computer 17 (schematically shown
in FIGURE 1 by a broken boundary line).

-14-

The transmitted ultrasonic signals from each transducer
propagate through the transmission medium until they
contact and bounce off of selected target tissue. The
reflected pulse/wave returns toward its transducer source

5   as an echo signal and is received by the transducer.
Echo signals, however, also will be received by adjacent
transducers but differences in the distance, properties
and noise characteristics of each transducer and
dispersion differences produced by layers of intervening

10 inhomogeneous medium will contribute to phase and
amplitude differences of the echo signal as received by
adjacent transducers. Individual transducers T_1 - T_N
will, therefore, receive the reflected echo signals over
a range of time delays corresponding to the position,

15 distance, contoured structure of the target and
reflectivity of the medium. The phase and amplitude of
the echo signal received by each transducer are measured
at each moment of time and input to computer 17 through
analog-to-digital converter 15.

20 Autocorrelator, diagrammatically indicated by box 14,
is adapted to autocorrelate the transmitted and received
signals for each transducer over the propagation time
delay. The autocorrelator executes a well-known
autocorrelation algorithm to perform an autocorrelation

25 between transmitted and received signals for each
transducer. Ideally and in applications other than
commercial ultrasonic echography, autocorrelator 14 is
coupled to a cross-correlator 16, shown in broken lines.
Cross-correlator 16 is adapted to cross-correlate pairs

30 of autocorrelated signals. The purpose of cross-
correlation is to determine the amplitude and phase
density distributions of the entire geometric aperture
defined by transducer bank 12. Cross-correlation
determines the phase offsets due to the relative physical

35 position differences between the cross-correlated pairs
of transducers relative to the target. These differences

-15-

are fixed as a result of the configuration of the transducer bank.

Commercial ultrasonic imaging equipment, however, does not currently include cross-correlation apparatus 16,
5   even though the use of such cross-correlation apparatus would eliminate phase aberration due to medium inhomogeneity. The artifact removal apparatus and process of the present invention, however, is applicable to image processing apparatus which includes cross-
10   correlation, as well as to apparatus which does not, such as conventional ultrasonic imaging equipment.

The amplitude and frequency data from autocorrelator 14 then can be directly stored as time domain data in data storage matrix 24 in the form of "visibility amplitude"
15   data, $A_{ij}{}^{\circ}$. Additionally, the "visibility phase" data is similarly stored directly in matrix 24 as time domain visibility phase data, $\phi_{ij}{}^{\circ}$.

These data alone often are used for image mapping, with the visibility phase data typically being discarded as
20   containing too much noise. My previous application described how additional useful data from ultrasonic imaging transducers can be obtained, partitioned and used for mapping, and such description is incorporated herein by reference. The apparatus and process of the present
25   invention for reducing data processing artifacts can be employed with various combinations of partitioned data as set forth in my prior application. It is not required, however, that my previous process for recovering additional useful data be employed in order
30   to practice the present invention for reducing data processing artifacts.

Briefly, however, additional data useful in image mapping can be obtained by a Fourier-like transformation at

-16-

Fourier transformer 18 which is coupled to autocorrelator
14. (If a cross-correlator 16 is employed, the output
of autocorrelator 14 is coupled to the cross-correlator,
which is then coupled to Fourier transformer 18.)
5   Fourier transformer 18 converts the time domain plots
of the array of transducers into the frequency domain
to yield spatial frequency data (U-V), which is used to
synthesize the beam and side lobe response for noise
deconvolution. The beam and side lobe response is
10 determined by assigning a two-dimensional position to
each   transducer   and   executing   a   Fourier-like
transformation of the array of delays to achieve a two-
dimensional spatial frequency spectrum characterized so
that each transducer pair corresponds to a (U-V) point.
15 Each U-V point is assigned its corresponding transducer
pair, and the representation of the U-V plane in the
Fourier transformed frequency domain yields the data to
be retransformed to produce the array point spread
function or "dirty beam." The Fourier transformed
20 frequency   domain   of   the   correlated   data   yields
information which can then be Fourier inverted to yield
a "dirty map." Such U-V data is stored in data storage
means or matrix 22.

Further useful data is obtained by a data partitioning
25 process for the visibility amplitude and visibility phase
data as well as the corresponding U-V data.

As can be seen at the center of FIGURE 1, visibility
amplitude data may be stored in memory storage matrix
26a, the visibility phase data in matrix 26b, and
30 "differential phase" data stored in matrix 26c. If a
cross-correlator 16 is present in the system, "closure
amplitude" data can be created and stored in matrix 26d
and "closure phase" data can be created and stored in
matrix 26e. U-V data indicating the beam and side lobe
35 response for the visibility and closure amplitudes and

phases and the differential phases are graphically shown
as stored in the corresponding sub-matrices. The
partitioned data can now be employed by mapper 27 to
produce an echographic image. While the data in matrices
5   26a-26e is significantly increased, it still contains
substantial noise, particularly in the phase data. Thus,
it is highly advantageous to employ further noise
reduction processing to enhance all data and particularly
the noisy phase data. As shown in FIGURE 1, the further
10 signal processing of the method of the present invention
takes the form of subtraction of the complex side lobe
noise inherent in a synthesized aperture, preferably by
using the CLEAN algorithm.

The next step in signal processing, therefore, is to
15 generate a "dirty" map of the area of the synthesized
aperture. The dirty map is defined as the Fourier
inversion of the visibility amplitudes and phases, and
if a cross-correlator is used, an inversion and modeling
of the closure amplitudes and phases. The dirty map
20 employs the frequency domain data in sub-matrices 26a-26e
using mapping techniques well known in the art. Mapper
27 will be understood to include a Fourier inversion
step, and the output of the mapper will be the original
dirty map data, which can be stored in data storage
25 matrix 29, and sent to identifier 36 and subtractor 34.

The dirty map produced will contain a high level of noise
produced by side lobe responses inherent to the multi-
transducer aperture array configuration. The side lobe
subtraction process uses the U-V data in matrices 26a-26e
30 to simulate a synthesized beam (a "dirty beam") response
of the transducer array to a single point source. The
dirty beam is the synthesized beam or point spread
function of the array. Beam synthesizer 40 is
responsible for converting or mapping the entire U-V data

-18-

into a beam power pattern in the frequency domain. The
beam power pattern which can be mapped from the U-V data
in effect represents the side lobes which would
inherently be generated if the target were a point
5   structure or source seen or viewed by array 12 of
transducers.

The side lobe subtraction or noise deconvolution process
is an iterative process, which may be practically
performed for real-time processing by using, but is not
10   limited to use of, the CLEAN algorithm.   It can be
performed in either the time or frequency domain, but
as illustrated in FIGURE 1, side lobe subtraction is
being performed in the time domain.

The first step is to identify the brightest point on the
15   dirty map by scanning the data with identifier means 36.
This identification is mathematically performed on the
data by looking at the greatest peak or highest intensity
value in the data. Since there are 262,144 data points
in a typical ultrasonic display (512 lines of 512
20   pixels), such as display 42, scanning the entire map for
the brightest point is computer burdensome.   One
technique which can be employed to reduce the computer
burden is to scan only each line of 512 pixels in the
X,Y or appropriately transformed image by identifier
25   means 36 on a line-by-line basis for the brightest data
point. If this technique is employed parallel processing
by identifier 36 can be used, with the identifier being
comprised of a plurality of parallel processors.

Once the brightest data point on the line (or map, if
30   not done line-by-line) is identified, the CLEAN algorithm
can be used to first deconvolve the point spread function
(dirty beam) from the remaining data on the line. In
the side lobe subtraction step the U-V beam response data
in beam synthesizer 40 for a point source is subtracted

from all the data in the line surrounding the brightest
or highest peak on the line, as indicated by subtractor
box 34 in FIGURE 1.   This step removes the data
representing side lobes around the bright point on the
5 line to yield a less noisy or "cleaner" map, with the
data which represents the side lobe response around the
bright data point being removed. Comparator 41 scans
or compares the data in the resulting line against
criteria as to the noise level which has been reduced.
10 Resolution input device 43, for example, can specify the
dynamic range of the map and lines therein, that is, the
range of maximum signal to the noise level. The dynamic
range can be required by input 43 to exceed a certain
amount or else the noise deconvolution process will
15 continue by going to the next brightest point on the
line.   Thus, if the criteria is not met, comparator 41
replaces the line data in mapper 27 with the cleaner data
and identifier 36 identifies the second brightest point
on the line so that subtractor 34 can remove the data
20 representing the side lobe response from all of the other
data on the line. This process continues until the data
in the line yields an acceptable outcome.

One assumption which must be made when doing a line-by-
line noise deconvolution is that the point spread
25 function or dirty beam is two-dimensional, not three-
dimensional. This assumption, however, is acceptable
because the side lobes tend to be negligible in extending
to the adjacent lines, particularly for the current
commercially marketed probes. With improved transducer
30 arrays side lobe data will begin to spill over or be
found in significant quantities in adjacent lines, which
will make line-by-line two-dimensional CLEAN subtractions
less acceptable, i.e., side lobes in adjacent lines will
be treated as being coupled or attached to data in the
35 line which they appear, instead of a bright point in the
adjacent line which actually caused the side lobe.

The problems introduced by the two-dimensional side lobe
subtraction, when the point spread function is three-
dimensional, can be greatly minimized by following the
two-dimensional CLEAN with a second two-dimensional

5   CLEAN, only with the data rotated by 90 degrees and the
point spread function modified to be a central high peak
and adjacent smaller side lobe peaks. Rotation of the
data and deconvolution of the rotated side peaks allows
the data representing side lobes in adjacent lines also

10 to be removed.

As indicated above, however, data being captured by
currently available ultrasonic apparatus will have a
point spread function or beam pattern which is very close
to two-dimensional, making line-by-line two-dimensional

15 deconvolution using the CLEAN algorithm highly effective
and a substantial reduction in computing burden.

During this iterative deconvolution process, a
significant amount of noise data will be removed from
the original data set which came from mapper 27 and now

20 is stored in data storage means 29. The side lobe
subtraction iteration, however, also will introduce into
the processed data set data points and values which do
not represent actual structure in the object being
imaged, i.e., processing artifacts. Accordingly once

25 comparator 41 senses that the dynamic range of the data
meets the criteria input, the data is passed to masking
means or "masker" 45 as a "processed data set."

The apparatus and process of the present invention
provide an accurate and yet simple system for removing

30 the processing noise component from the processed data
set. Masking means 45 accomplishes this end by
multiplying the values of data (the pixel intensity
values) in the processed data set (map) by the values
of corresponding data (pixel intensity values) in the

original data set (map). Thus, each pixel intensity
value in the processed map is multiplied by the
corresponding pixel intensity value in the dirty map.
The processed data set from comparator 41, which is
5   passed to masking means 45, is multiplied times
corresponding data from the dirty map in storage means
29 on a pixel by pixel basis. This revaluing or masking
of data is a form of what is sometimes referred to as
"self-apodization."

10   Original or "dirty" map data as stored in storage means
29 includes all of the valid data from the original data
set to accurately reproduce the image. The data in
storage means 29 also includes a substantial amount of
noise data which does not represent valid target
15   structure. The data which is passed from comparator 41
to masking device 45 has eliminated a substantial amount
of the noise which is present in the data in storage
device 29, but it also has introduced a much smaller
quantity of processing noise or artifacts. The effect
20   of multiplying corresponding data values for the dirty
map times the noise-reduced map is that data which is
present in both data sets will be reinforced in the data
sent to normalizer 39, while the processing noise
component data which was introduced after the dirty map
25   was generated will have no corresponding reinforcement
by the dirty data in storage device 29. The dirty data
in storage device 29, therefore, has the effect of
masking out or removing the processing noise component
of the data in the processed data set.

30   If the original image data set includes zero pixel value,
intensity multiplying processed image data by zero will
have the effect of discarding data in the processed image
data set which was not also present in the original image
data set. For low value data in the original image data
35   set, the low value of such data when multiplied times

-22-

the corresponding processed image data will reduce the
value of artifacts which are coincidentally present.

It will be appreciated that it is statistically possible
for the processing noise component of the processed data
5   set to have some artifacts which are coincidental with
noise in the original dirty data set. Thus, the masking
process of the present invention may not eliminate all
of the processing noise component in the processed data
set, but it will effect a substantial reduction in such
10 noise component and statistically can also effect
complete elimination of the processing noise component
in certain instances.

In more complex imaging processing systems, and
particularly those not requiring real-time display, it
15 would even be possible to employ double masking. For
example, the data can be processed using side lobe
subtraction followed by masking to reduce the processing
noise component. The same data can then be processed
using hybrid mapping or maximum entropy and masked to
20 reduce the processing noise component. These two sets
of data can then be masked against each other so that
only the data points which are common to both data sets
are reinforced and the non-common ones are masked out.
This will further reduce the noise by reducing
25 statistically coincident processing noise components
because the two differing signal processing techniques
will produce differing artifacts that will have differing
statistical coincidences with data in the original or
dirty data set.

30 The preferred technique for multiplying the values in
the processed data set by the values in the original data
set is to multiply the value of data in the processed
image data set by the absolute value of corresponding
data in the original image data set and then to divide

that result by the highest data value of any data in the
original image data set. This division step has a
scaling effect so that data values do not exceed a
maximum.

5   The reduction of noise from processed image data of the
present invention is particularly useful for noise
reduction processes such as side lobe subtraction using
a CLEAN algorithm, maximum entropy noise reduction and
hybrid mapping noise reduction. It can be used when the
10   data is captured by radar imaging apparatus, sonar
imaging apparatus, microwave imaging apparatus,
ultrasonic imaging apparatus, optical imaging apparatus
and radio astronomy imaging apparatus, as long as the
captured image data has been processed by an image
15   processing technique which introduces a processing noise
component. Since revaluing the data to eliminate or
reduce the processing image component is merely a
multiplication, usually in combination with a division
for scaling, the process of the present invention is not
20   computer burdensome nor does it prevent real-time
processing.

Before data masking has been effected, the data is passed
to convolver or convolving means 46. The CLEAN algorithm
is preferably again used on a line-by-line basis to
25   convolve a two-dimensional side lobe-free point spread
function or "clean beam" back into the deconvolved and
noise-reduced data prior to masking of the data.

One technique which can be used to further enhance the
resolution of the displayed image is to use the CLEAN
30   algorithm to control the restoring or clean beam to a
width substantially smaller than that of the main lobe
on the dirty beam. This is an "over-processing" of the
data, but it is very acceptable and achieves super-
resolution in ultrasonic applications. Thus, the CLEAN

algorithm can be used to narrow the side lobe-free point
spread function as it is convolved by convolver 46 back
into the data to masking device 45. When you narrow the
restoring or clean beam you increase the effective
5   diameter of the aperture. It will be appreciated,
however, that as the restoring beam is narrowed, you
begin to "eat away" or create holes in the data, i.e.,
overprocessing. Nevertheless resolution of the images
increases and such overprocessing can proceed, for
10 example, past the Rayleigh's criteria, which is referred
to as "superresolution."

One effect of the masking process of the present
invention is that the contrast can be increased as a
result of pixel intensity revaluation to a degree which
15 arguably can hide real target features. It is a further
important feature of the present invention that
normalizing be provided to normalize the intensity or
prevent undesirable contrast changes.

This normalization can be effected at normalizer 39 by
20 applying the n^{th} power to the data values, rather than
forming a display image from the values after the masking
revaluation step. If the brightest point on the data
map or line has a value of 1.0, the n^{th} power of that
value also is equal to 1.0. The powers preferred are
25 between about 0.2 and 1.0. Thus, the square root (n =
0.5) of a data point having a value of 0.49 is 0.7, which
effectively causes the intensities to converge toward
the brightest point and the contrast differences to be
reduced.

30 As will be appreciated if one wanted to increase the
contrast for any reason, a converse process could be
employed, namely, use and display masked data taken to
a power greater than 1.0, e.g., n = 2. Again, a data

value of 1.0 would remain unchanged while a value of 0.5
would decrease to 0.25.

It should be noted in this regard that most ultrasonic
display devices 42 are capable of generating pixels
5 commonly having 64 or 256 intensity gradations, with zero
being black and 64 or 256 being the highest intensity.
The values after masking will range from zero to 1.0 and
they are accordingly attributed to the range of intensity
levels available on the video display.

10 In a second aspect of the process and apparatus of the
present invention correction for phase aberration or near
field effects is provided. As above noted the provision
of a cross-correlator 16 and partition of the data to
include closure amplitude and closure phase data (storage
15 means 26d and 26e) will completely eliminate the problem
of phase aberration caused by transmission and/or receipt
of signals through inhomogeneous mediums. Unfortunately,
commercially available ultrasonic imaging apparatus does
not include cross-correlation apparatus. It is a purpose
20 of the present invention, therefore, to effect a
reduction in the phase aberration in image processing
equipment which does not include or use cross-correlation
to eliminate phase aberration.

Referring now to FIGURE 2A and 2D, a graphical
25 representation of a hypothetical image data set is shown
as it would be seen if displayed from memory at various
stages of processing using the signal processing method
of my prior application. Thus, graphical representation
61 shows the image data in polar coordinates, r, θ.
30 Medical personnel are used to viewing ultrasonic image
data in a polar format, rather than a Cartesian format.
Video display tubes are physically constructed with
Cartesian screens, that is lines and rows of pixels, but
the image on graph 61 would have the same shape as shown

on a video display 42, except that the pixel grid would
be Cartesian.

In polar data graph 61 there will be seen to be a
plurality of solid grid "squares" that represent actual
5   or real image data.   This is the data that imaging
personnel want to see, and it is shown again in FIGURE
2C as graph 62.   In polar graph 61, however, there is
phase aberration data, shown by squares with an "X"
inside them, and there is noise data, shown by squares
10   with a "O" inside them. If graph 61 was to be displayed
without processing, a very cloudy image would be seen
in which it would be difficult to determine the real
shape of the target, namely, graph 62.

Accordingly, to facilitate side lobe subtraction using
15   the CLEAN algorithm, or other signal processing
techniques, the r,θ data captured by the transducer array
is usually converted into Cartesian or X,Y data, as shown
at screen 63 in FIGURE 2A. As will be seen by comparison
of graphical representations 61 and 63, all the data is
20   still present in graph 63 that was present in graph 61.

While it is conventional to perform the CLEAN
deconvolution in a Cartesian coordinates, rather than
polar coordinates, it should be noted that it also is
possible to use a coordinate transformation of the point
25   spread function or beam and then perform the CLEAN in
r,θ or polar coordinates. In either approach, however,
a transformation between coordinate systems must be
undertaken.

The coordinate transformation so as to produce exactly
30   equivalent Cartesian coordinates from polar coordinates,
or vice versa, is covered by simple algorithm, namely:

-27-

$$r = \sqrt{(X-K_x)^2 + (Y+K_y)^2}$$

$$\theta = \arctan\left(\frac{X-K_x}{Y+K_y}\right)$$

where K_x and K_y are constants dependent upon the distances from r=0 and θ=0 to X=0 and Y=0.

If the conventional above set forth coordinate transfer is used, the phase aberration data in the image data set,
5   caused by transmission of the signal and its reflection through an inhomogeneous medium will simply be passed through to graph 61, as will all noise data.

The next step in data processing is to remove the side lobes, for example, by use of the CLEAN algorithm. As
10   will be seen from graph 64, therefore, the noise data has been removed using the CLEAN algorithm in Cartesian coordinates. As also can be seen in graph 64, the CLEAN signal processing step has introduced a few processing artifacts, the data represented by a triangle inside the
15   data squares.

The X,Y or Cartesian data after the CLEAN step can then be converted back to r,θ, or polar, coordinates for display. Thus, graph 66 illustrates the image which would be displayed after signal processing using the
20   process of my prior application without cross-correlation, and it can be seen to include phase-aberration or near-field effect data. It should be noted again that the same data image as shown on graph 66 would be displayed on a Cartesian screen so that the video
25   screen 42 would have an X,Y grid, but the image would have the appearance of screen 66, not screen 64.

-28-

In the process and apparatus of the present invention,
however, a coordinate transformation input device 55
(FIGURE 1) can be used to input the data processor or
computer 17 with non-standard coordinate transfer
5   algorithms. (As will be appreciated input device 55 and
input device 43 can be provided by a convention computer
input device such as a key board.) Such non-standard
coordinate transfer algorithms have the effect of
distorting the data and resultant image. Such distortion
10 can be used to counter or compensate for the effect of
phase aberration by reason of passage of the signals
through an inhomogeneous medium.

Coordinate transformation input device 55, therefore,
can be used to vary the coordinate transformation
15 algorithms in a manner which is empirically determined
for standard medical applications to correct for phase
aberration which typically occurs in such applications.
In transabdominal ultrasonic imaging, for example, one
will experience a different amount and type of phase
20 aberration than occurs in transvaginal applications.
Input device 55 can be used to vary the coordinate
transformation algorithms while viewing the resulting
image. A table can be established, therefore, as to
which variations produce greater resolution and which
25 variations produce image blurring. Ultimately, such a
comparison system can be done computationally in computer
17 with means being provided to compare image resolution
against an input criteria and to automatically vary the
coordinate transformation algorithms until the highest
30 degree of resolution is achieved.

In FIGURE 2B, graph 67 is identical to graph 61 and
contains real image data, phase aberration data and noise
data. At the step represented by box 68, a non-standard
coordinate transformation takes place through input from
35 input device 55. As will be seen, the data of graph 67

-29-

has been transformed to data on a distorted "Cartesian" grid 69, with the result that the area occupied by the data has been changed. Again, all the data are present in graph 69, but it has been compressed and skewed as
5   a result of the non-standard coordinate transformation.

Graph 69 illustrates a two dimensional proportional non-standard coordinate transformation. It will be understood, however, that non-standard coordinate transformations can be one or two-dimensional and can
10   be localized.

At step 71 the data in graph 69 has been subject to a CLEAN side lobe subtraction, which eliminates the noise data, and has been masked, which eliminates the processing artifacts. The result is shown on graph 72
15   in which the data is shown on a standard Cartesian coordinate grid, but it has been distorted in shape to the shape of the data in grid 69, less the noise data, eliminated by the CLEAN, and without any artifact data, eliminated by the masking. The number of "data points"
20   appears to be less in graph 72 than in graph 69 by reason of plotting on the undistorted Cartesian graph, but the shape and area of the real data and phase aberration data are substantially the same (changed only by the size of the grid and large size of the squares which require a
25   graphical approximation). Finally, the CLEANed and masked data is returned to polar coordinates in graph 73 in a standard coordinate transformation preparatory to display on video output device 42. As will be seen by comparing graphs 62, 66 and 73, the image which would
30   be displayed from the data in graph 73 is much closer to the ideal image of graph 62 than is the image of graph 66. The graph 73 image has not eliminated the phase-aberration data, but instead it has been distorted in a manner compensating for the distortion produced by the
35   inhomogeneous medium.

This phase aberration approximation is not an exact solution to phase aberration, as is cross-correlation, but it does provide a system in which medical personnel can try various coordinate transformations as a way of
5   clearing or reducing phase aberration. Since the computational burden is not great, such empirical adjustment, particularly with the aid of tables, can be accomplished by the physician or technician during real-time imaging. The technique of the present invention
10 is somewhat analogous to dropping different lenses in front of the transducer array to reduce phase aberration without cross-correlation.

-31-

WHAT IS CLAIMED IS:

1.   A method of producing an image of an object having
a reduced noise component comprising the steps of:
        positioning imaging transducer means for receipt
5   of a sufficient number of image signals from said object
to permit an image of said object to be produced;
        transforming said image signals into an original
data set;
        processing said original data set by a noise
10 deconvolving process producing a processed data set in
which said noise component is reduced as compared to said
original data set and a processing noise component has
been introduced into said processed data set;
        thereafter reducing said processing noise component
15 in said processed data set by multiplying the value of
individual data in said processed data set by the value
of corresponding individual data in said original data
set; and
        thereafter displaying data resulting from said
20 reducing step as an echographic image.

2.   A method of clinically analyzing a physical
condition comprising the steps of:
        transmitting ultrasonic signals from transducer
means into a patient's tissues;
25   receiving echo signals by transducer means from said
tissues to provide an original image data set of signals
of said tissues;
        processing said original image data set of signals
to produce a processed image data set of signals having
30 reduced noise components and artifact data;
        revaluing at least some of the data in said
processed image data set of signals by an amount
proportional to the value of corresponding data in said
original image data set of signals;

-32-

after said revaluing step, displaying the data in said processed image data set as a noise-reduced image; and

5   thereafter using the image created during said displaying step to clinically analyze said tissues.

3.   The method as defined in claim 2 wherein, said revaluing step is accomplished by valuing as zero all non-zero value data in said processed image data set for which corresponding data in said original image

10   data set has a zero value.

4.   The method as defined in claim 2 wherein, said revaluing data step is accomplished by discarding all data in said processed image data set not also present in said original image data set.

15   5.   The method as defined in claim 2 wherein, said revaluing step is accomplished by multiplying the value of data in the processed image data set by the value of corresponding data in said original image data set.

20   6.   The method as defined in claim 2 wherein, said revaluing step is accomplished by multiplying the value of data in said processed image data set by the absolute value of said corresponding data in said original image data set and dividing the product by the

25   highest data value of any data in said original image data set.

7.   The method as defined in claim 6, and the step of: after said revaluing step, normalizing the value of said data in said processed image data set by raising

30   the value of said data in said processed image data set to the power n, where n is between about 0.2 to about 1.0.

-33-

8.   The method as defined in claim 2 and the step of:
      after said revaluing step, raising each data value
in said processed image data step to a power between
about 0.2 and about 1.0.

5   9.   The method as defined in claim 2 and the step of:
      producing said processed image data set by
deconvolving the original noise component from said
original image data set and eliminating at least a
portion of said noise component.

10 10.   The method as defined in claim 9 wherein,
      said producing step is accomplished by at least one
of the processes of:
      a CLEAN deconvolution, a maximum entropy
deconvolution, and a hybrid mapping deconvolution.

15 11.   A method of enhancing the dynamic range of an image
produced from data in an original image data set
comprising the steps of:
      positioning an imaging transducer for receipt of
a sufficient number of image signals from an object to
20 be imaged to provide said original image data set;
      processing said original image data set by a signal
processing technique producing a processed image data
set including image data having an enhanced dynamic range
relative to said original image data set and including
25 artifact image data produced by said processing
technique; and
      reducing the quantity of artifact image data in said
processed image data set to further enhance dynamic range
by multiplying the value of at least a portion of the
30 data in said processed image data set by the value of
corresponding data in said original image data set.

12.   The method as defined in claim 11 wherein,
said step of processing is accomplished by
processing an original image data set obtained from
echographic imaging apparatus.

5 13.   The method as defined in claim 12 wherein,
said echographic imaging apparatus is an ultrasonic
imaging apparatus.

14.   The method as defined in claim 12 wherein,
said echographic imaging apparatus is a radar
10 imaging apparatus.

15.   The method as defined in claim 12 wherein,
said echographic imaging apparatus is a sonar
imaging apparatus.

16.   The method as defined in claim 12 wherein,
15   said echographic imaging apparatus is a microwave
imaging apparatus.

17.   The method as defined in claim 11 wherein,
said step of processing is accomplished by
processing an original image data set obtained from radio
20 astronomy imaging apparatus.

18.   An imaging apparatus comprising:
an array having a plurality signal receiving
transducers formed for receipt of a sufficient number
of image signals from an object to be imaged to enable
25 creation of an image display therefrom;
processing means coupled to said array and
responsive to receipt of said imaging signals to
transform said imaging signals into an original data set
containing a noise component resulting from use of said
30 array to receive said image signals, said processing
means and processing said original data set to produce

a processed data set having a reduced original noise component and a processing noise component;

data valuation means coupled to said processing means and responsive to production of a processed data
5   set to revalue data in said processed data set by multiplying the value of data in said processed data set with the value of data in said original data set to reduce said processing noise component from said processed data set; and

10   display means connected to display data multiplied by said data valuation means as an image of said object.

19.   The data processing apparatus as defined in claim 18 wherein,

said data acquisition means is an image data
15 acquisition means.

20.   The data processing apparatus as defined in claim 19 wherein,

said image data acquisition means is an echographic imaging apparatus.

20 21.   The data processing apparatus as defined in claim 20 wherein,

said echographic imaging apparatus is an ultrasonic imaging apparatus.

22.   The data processing apparatus as defined in claim 20
25 wherein,

said echographic imaging apparatus is a radar imaging apparatus.

23.   The data processing apparatus as defined in claim 20 wherein,

30   said echographic imaging apparatus is a sonar imaging apparatus.

24. The data processing apparatus as defined in claim 20 wherein,

said echographic imaging apparatus is a microwave imaging apparatus.

5   25. The data processing apparatus as defined in claim 19 wherein,

said image data acquisition means is a radio astronomy imaging apparatus.

26. An echographic imaging apparatus comprising:
10   transducer means formed to produce transmitted signals which can be directed against an imaging target and formed to receive echo signals including a noise component from said target;

first signal processing means coupled to said
15   transducer means and response to receipt of said echo signals by said transducer means to transform said transmitted signals and said echo signals into an original image data set having an original noise component;

20   second signal processing means coupled to said first signal processing means and response to production of said original image data set to produce a processed image data set in which said original noise component is reduced and a processing noise component has been
25   introduced;

data valuation means coupled to said second image processing means and responsive to production of said processed signal data set to multiply the value of data in the processed image data set by the value of
30   corresponding data in the original image data set to reduce said processing noise component in said processed image data set; and

display means connected to receive data multiplied by said data valuation means and formed to display the
35   multiplied data as an echographic image.

-37-

27. The apparatus as defined in claim 26 wherein,
      said data valuation means is further responsive to
said comparison by said comparator means to divide the
product of the value of data in said original image data
5 set times the value of corresponding data in said
processed image data set by the highest value of any data
in said original image data set.

28. The apparatus as defined in claim 27 wherein,
      said data valuation means includes normalization
10 means responsive to input of revolved data to raise the
value of said revolved data to a power between about 0.2
to about 1.0.

29. The apparatus as defined in claim 27 wherein,
      said transducer means produces ultrasonic signals.

15 30. The apparatus as defined in claim 27 wherein,
      said transducer means produces radar signals.

31. The apparatus as defined in claim 27 wherein,
      said transducer means produces sonar signals.

32. The apparatus as defined in claim 27 wherein,
20   said transducer means produces electromagnetic
signals.

33. A method producing an image of an object having
reduced phase aberration comprising the steps of:
      positioning transducer means for receipt of image
25 signals from said object through an inhomogeneous medium
located between said transducer means and said object;
      transforming said image signals into an image data
set expressed in one of a polar and Cartesian coordinate
system;
30   performing a coordinate transformation between said
one of said polar and Cartesian coordinate system and

the remainder of said polar and Cartesian coordinate
system using a modified coordinate transformation
algorithm set on one of:

        (i)   data from said image data set, and

5   (ii) a noise deconvolution algorithm; and
displaying an image produced from a data set after said
step of performing a coordinate transformation has been
accomplished.

34.   The method as defined in claim 33 wherein,
10   said step of performing a coordinate transformation
is accomplished by performing said transformation on data
from an image data set and is followed by a noise
deconvolution process.

35.   The method as defined in claim 34 wherein,
15   said data is collected in polar coordinates and said
transformation step converts said data to modified
Cartesian coordinates.

36.   The method as defined in claim 35 wherein,
    after said deconvolution step, transforming
20 deconvolved data from a modified Cartesian system to a
polar coordinate system using a standard coordinate
transformation algorithm set.

37.   The method as defined in claim 33 wherein,
    said step of performing a coordinate transformation
25 step is accomplished after collection of data and prior
to a noise deconvolution process.

38.   The method as defined in claim 36 wherein,
    said transformation step is accomplished by
transformation of a deconvolution algorithm from a
30 Cartesian coordinate system to a modified polar
coordinate system.

39. The method as defined in claim 33 wherein,
     said modified coordinate transformation algorithms
are empirically selected to correct for signal distortion
in an inhomogeneous medium.

5 40. The method as defined in claim 33 and the step of:
     after said transformation step, deconvolving noise
from said image data; and
     after said deconvolving step, removing deconvolving
artifacts from said image data set by a self-apodization
10 process in which the value of individual data points from
the deconvolved data set is multiplied by the value of
corresponding individual data in said image data set.

41. The method as defined in claim 40, and the
additional step of:
15   after the step of multiplying the value of said
deconvolved data set by corresponding data values in said
image data set, dividing the products by the value of
the highest data value in the image data set, and
thereafter raising the quotients to a power between about
20 0.2 and about 1.0.

42. The method as defined in claim 33 wherein,
     said step of performing a coordinate transformation
is accomplished on autocorrelated data expressed in polar
coordinates.

25 43. The method as defined in claim 33, and the steps
of:
     prior to said performing step, displaying said image
data and visually inspecting the displayed image for
phase aberration noise;
30   thereafter selecting a first set of modified
coordinate algorithms prior to said step of performing
a coordinate transformation, and

after said step of performing a coordinate transformation, displaying the modified image date to visually determine the effect of the selected modified coordinate algorithms on phase aberration; and

5   after said step of displaying the modified image data, selecting a second set of modified coordinate algorithms having values different from said first set by an amount selected to reduce phase aberration, and performing said coordinate transformation a second time

10 using said second set of modified coordinate algorithms, and displaying the image resulting therefrom.

44. An apparatus for the reduction of phase aberration error from an image data set produced by echographic imaging apparatus comprising:

15   coordinate transformation means coupled to said echographic imaging apparatus and responsive to production of said image data set by said echographic imaging apparatus to change the coordinate system between polar and Cartesian coordinates for one of image data

20 and a noise deconvolution algorithm, said coordinate transformation means changing between coordinate systems by applying a coordinate transformation algorithm set thereto which differs from a conventional coordinate transformation algorithm by an amount tending to reduce

25 phase aberration in said image data set.

45. An apparatus as defined in claim 44 wherein, said coordinate transformation means includes user input means for user input to effect a selection of the modified coordinate transformation algorithm set.

30 46. An apparatus as defined in claim 45 wherein, said coordinate transformation means performs a coordinate transformation of input data from polar to Cartesian coordinates using said modified transformation algorithm set.

47. A method of generating an echographic image of a target object comprising the steps of:

(a) transmitting a plurality of ultrasonic signals toward said target object using a signal generating
5 assembly;

(b) receiving a corresponding plurality of echo signals from said target object with signal receiving transducer means;

(c) in response to receipt of said echo signals
10 correlating said ultrasonic signals and said echo signals using correlation means to produce correlated data including at least one of amplitude data and phase data sufficient to map an image of said target object; and

(d) reducing noise present in said correlated data
15 by signal processing means by at least one of: (i) a side lobe subtraction process, (ii) a hybrid mapping process, (iii) a vectorial summing process, (iv) a ratio forming process, and

(e) mapping at least one of said amplitude data
20 and said phase data after said step of reducing noise.

48. The method of generating an echographic image of a target object as defined in claim 47, and

prior to said noise reducing step, partitioning said correlated data by partitioning means into a plurality
25 of data sets including at least one of a visibility amplitude data set and a visibility phase data set.

49. An apparatus for generating an echographic image comprising:

a plurality of ultrasonic transducers mounted in
30 an array,

generator means coupled to drive said transducers,

signal processing means coupled to said transducers to receive echo signal data therefrom and coupled to receive transmitted ultrasonic signal data, said signal
35 processing means correlating and mapping at least one

of amplitude data and phase data from said ultrasonic signal data and said echo signal data, said signal processing means including means for processing at least one of amplitude data and phase data including means for

5   reducing noise in at least one of said amplitude data and said phase data, said means for reducing noise being provided by one of: (i) means for subtracting side lobe noise from said one of said amplitude data and said phase data, and (ii) means for substituting hybrid map data

10   for one of actual phase data and actual amplitude data, and said signal processing means further including mapping means for mapping at least one of said amplitude data and said phase data after the reduction of noise therefrom; and

15   display means coupled to said signal processing means to receive mapped data from said signal processing means and to display said mapped data in an image.

50. An apparatus for generating an echographic image comprising:

20   a plurality of ultrasonic transducers mounted in an array;

         signal generator means coupled to drive said transducers;

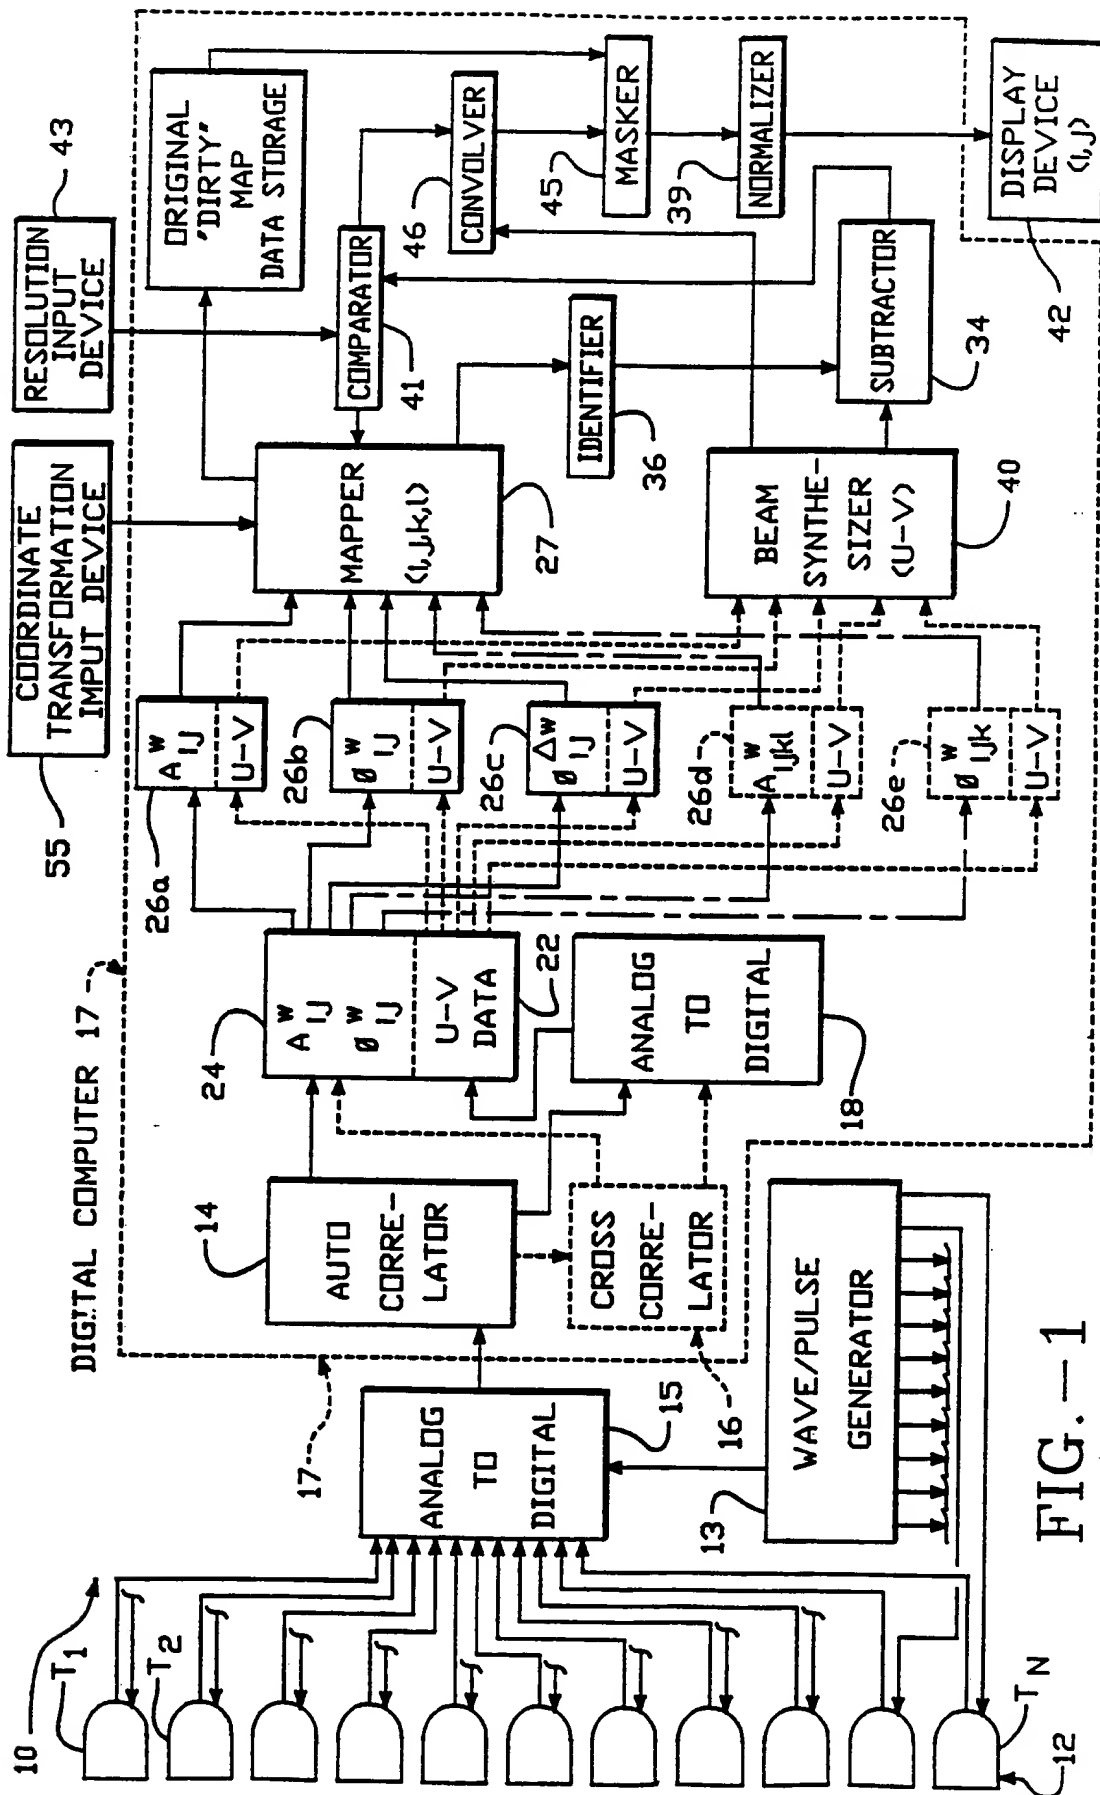   signal processing means coupled to receive echo

25   signals from said transducers and coupled to receive echo signals, said signal processing means being responsive to correlate said echo signals relative to said transmitted signals to produce at least one of phase signals and amplitude signals suitable for image mapping,

30   said signal processing means further including noise reduction means responsive to at least one of said phase signals and said amplitude signals to reduce noise in said one of said phase signals and said amplitude signals;

35   said noise reduction means including at least one of:

-43-

(i) means for subtracting said lobe noise from at least
one of said amplitude signals and said phase signals,
(ii) means for substituting hybrid map signals for at
least one of said amplitude signals and said phase
5   signals, (iii) means for vectorially summing sets of
three phase signals to produce closure phase signals,
and (iv) means for forming ratios of sets of four
amplitude signals to produce closure amplitude signals;
and

10   display means coupled to said signal processing
means to receive at least one of said phase signals and
said amplitude signals after noise reduction by said
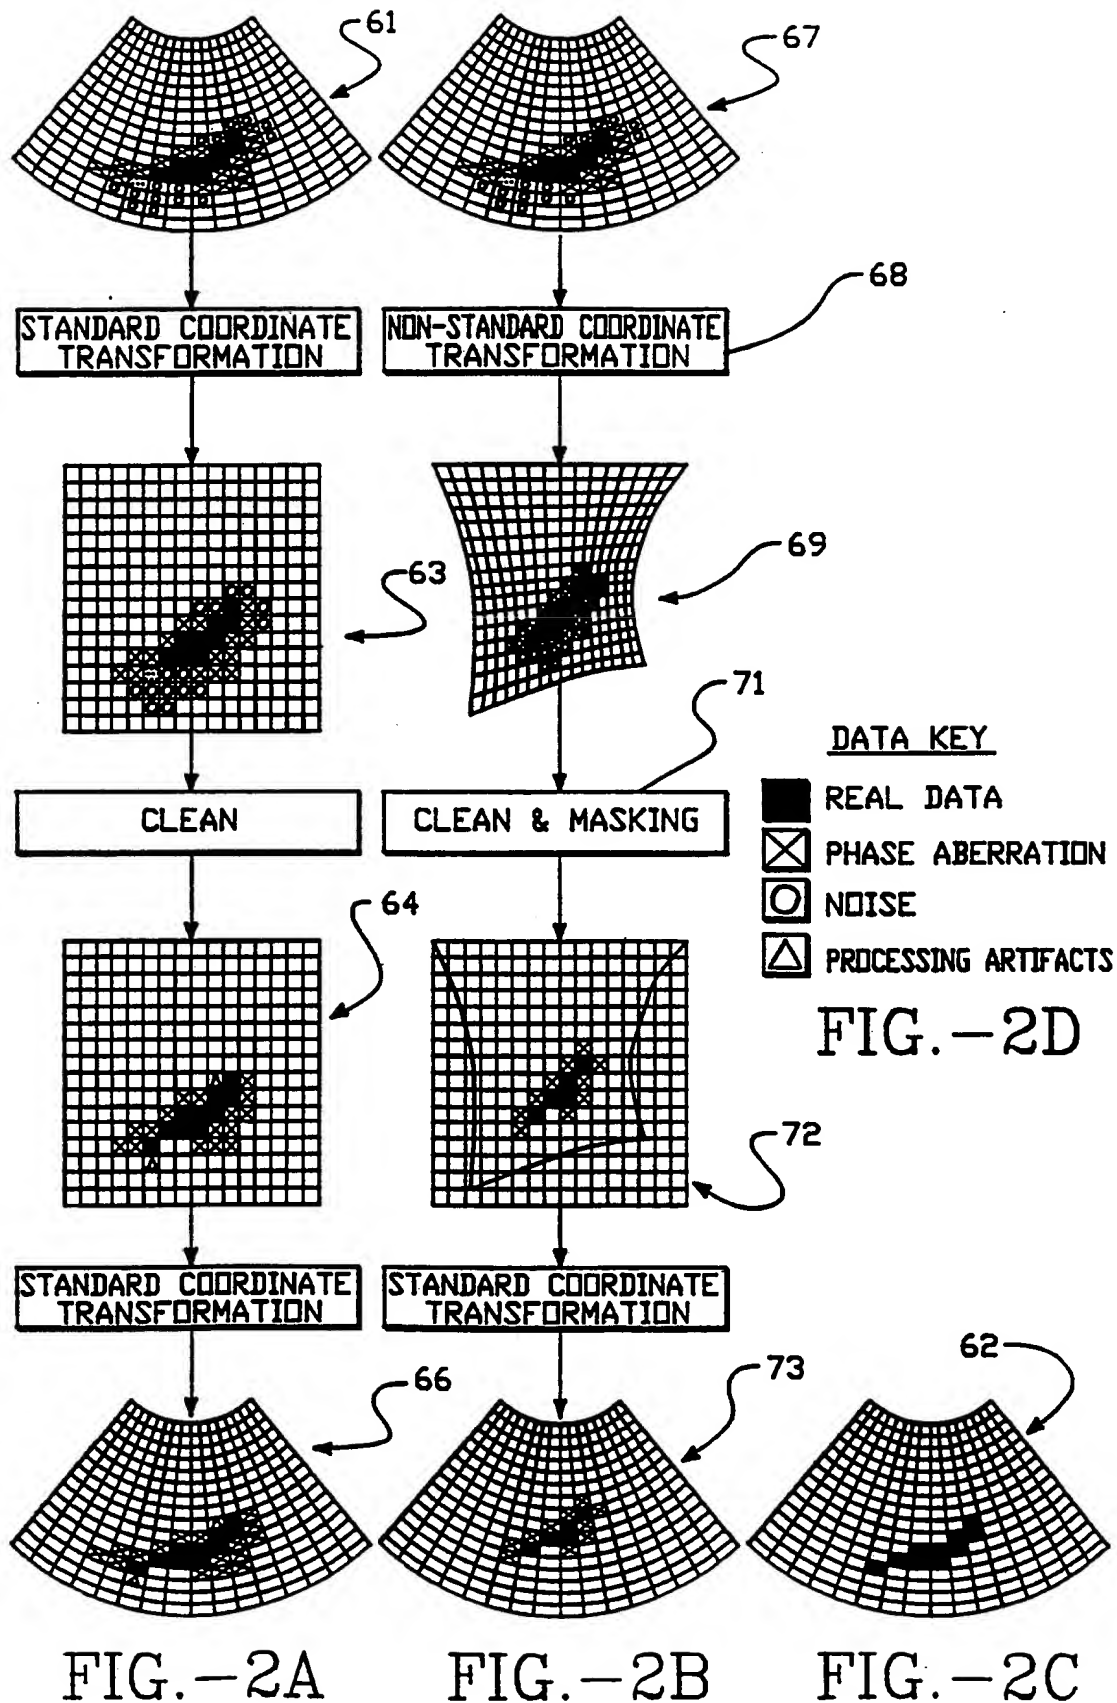noise reduction means and responsive thereto to produce
an image.

FIG. -1

FIG.—2A   FIG.—2B   FIG.—2C

FIG.—2D

DATA KEY

■ REAL DATA
⊠ PHASE ABERRATION
⊙ NOISE
△ PROCESSING ARTIFACTS

INTERNATIONAL SEARCH REPORT

A. CLASSIFICATION OF SUBJECT MATTER

IPC(5) :A61B 8/00
US CL :128/660.07

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 364/413.25 73/602,625,626 342/25,145,179,203,379

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X,P	US,A, 5,105,814 (Drukarey et al.) published 21 April 1992, See column 6 line 47-column 7 line 4.	2
Y	US,A, 4,397,006 (Galbraith, Jr.) published 02 August 1983, see column 3 lines 3-31.	2
Y,E	US,A, 5,197,037 (Leavitt) published 23 March 1993 see column 2 lines 6-11.	33,35,37,44
Y,P	US,A, 5,111,823 (Cohen) published 12 May 1992 See abstract.	47-50

☐ Further documents are listed in the continuation of Box C.   ☐ See patent family annex.

*	Special categories of cited documents:	"T"	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A"	document defining the general state of the art which is not considered to be part of particular relevance		
"E"	earlier document published on or after the international filing date	"X"	document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"L"	document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)		
		"Y"	document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"O"	document referring to an oral disclosure, use, exhibition or other means		
"P"	document published prior to the international filing date but later than the priority date claimed	"&"	document member of the same patent family

Date of the actual completion of the international search	Date of mailing of the international search report
08 APRIL 1993	07 JUN 1993
Name and mailing address of the ISA/US Commissioner of Patents and Trademarks Box PCT Washington, D.C. 20231	Authorized officer FRANCIS J. JAWORSKI
Facsimile No. NOT APPLICABLE	Telephone No. (703) 308-0858

Form PCT/ISA/210 (second sheet)(July 1992)*